
Master Agreement - E194 - 441 - 1

Document Id: 441

Document Name: Patient Lift/Transfer Systems
& Access.

Print Date: 2/2/2007

Procurement Folder: 758

Procurement Type: IFB

Effective Begin Date: 2/2/2007

Expiration Date: 7/31/2009

Issuer Name: Tina Mizelle

Phone: (804) 786-1603

Email: tina.mizelle@dgs.virginia.gov

Document Description: **Patient Lift/Transfer Systems & Accessories**

Created By: tmizelle1

Modified By: tmizelle1

Created On: 2007-02-02

Modified On: 2007-02-02

Contact Information

Tina Mizelle

Phone: (804) 786-1603

Email: tina.mizelle@dgs.virginia.gov

Thresholds

Minimum Order Amount: \$0.00

Minimum Order Value: Yes

Maximum Order Amount: \$0.00

Maximum Order Value: No

Authorized Departments

All Commonwealth of Virginia State Agencies, Commissions, Authorities, Boards, Public Bodies and other Entities Authorized by the *Code of Virginia*.

Vendor

Legal Name: **MasterCare Patient Equipment, Inc.**

Vendor Contact Name: Diane Walkowiak

Location Legal Name: Columbus, NE

Vendor Contact Email:

mastercarepeinc@yahoo.com

Vendor Contact Phone: 800-798-5867

Vendor Type: Primary

MA Number: E194 - 441

Renewal Periods

Line Number: 1

Renewal Period Length: 1

Renewal Period Unit: Years

Effective Date: 8/1/2009

Expiration Date: 7/31/2010

Notification Days Prior to Expiration: 90

Line Number: 2

Renewal Period Length: 1

Effective Date: 8/1/2010

Notification Days Prior to Expiration: 90

Renewal Period Unit: Years

Expiration Date: 7/31/2011

Line Number: 3

Renewal Period Length: 1

Effective Date: 8/2/2011

Notification Days Prior to Expiration: 90

Renewal Period Unit: Years

Expiration Date: 8/1/2012

Terms and Conditions

Section 04

EVA BUS TO GOV CONTRACT PART 1

eVA BUSINESS-TO-GOVERNMENT CONTRACTS: The eVA Internet electronic procurement solution, web site portal www.eva.state.va.us, streamlines and automates government purchasing activities in the Commonwealth. The portal is the gateway for vendors to conduct business with state agencies and public bodies. Failure to comply with the requirements in a. and b. below will be just cause for the Commonwealth to reject your bid/offer or terminate this contract for default. Vendors desiring to provide goods and/or services to the Commonwealth shall participate in the eVA Internet e procurement solution and agree to comply with the following:

Section 05

EVA BUS TO GOV CONTRACT PART 2

A. Submit a fully executed American Management Systems, Inc., (AMS) Trading Partner Agreement, a copy of which can be accessed and downloaded from www.eva.state.va.us. AMS is the Commonwealth's service provider to implement and host the eVA e-procurement solution. B. Provide an electronic catalog (price list) for items awarded under a term contract. The format of this electronic catalog shall conform to the eVA Catalog Interchange Format (CIF) Specification that can be accessed and downloaded from www.eva.state.va.us.

Section 06

CONTRACT TERM

THE INITIAL TERM OF THIS CONTRACT WILL BE FOR TWO YEARS BEGINNING APPROXIMATELY June 9, 2006 through July 31, 2008.

Section 07

RENEWAL OF CONTRACT

This contract may be renewed by the Commonwealth upon written agreement of both parties for three (3) additional successive one (1) year periods under the terms and conditions of the current contract, and at a reasonable time (approximately 90 day) prior to expiration.

Section 08

AWARD

The Commonwealth will make multiple awards by manufacturers' product lines, on a GRAND TOTAL basis to the lowest responsive and responsible Bidders. The number of awards is entirely at the discretion of the Commonwealth. The purchasing office reserves the right to conduct any test it may deem advisable to make all evaluations. The Commonwealth also reserves the right to reject any or all bids, in whole or in part, to waive informalities and to delete items prior to making the award, whenever it is deemed in the sole opinion of the procuring public body to be in its best interest.

Section 10

BID ACCEPTANCE PERIOD

Any response in reply to this solicitation shall be valid for 60 days. At the end of the 60 days the response may be withdrawn by the Vendor upon written request. If it is not withdrawn at that time, it remains in effect until an award is made or the solicitation is cancelled.

Section 13

DELIVERY SERVICE

Delivery of all requested contract items shall be made within 3 to 6 weeks after receipt of purchase order. Contractor shall carry an adequate stock to insure such delivery service for the duration of the contract.

Section 14

DELIVERY / SHIPPING POINT

Except when otherwise specified herein, all items shall be F.O.B. destination delivered any point within the Commonwealth of Virginia as directed by ordering department, institution or agency of the Commonwealth or Public bodies of the Commonwealth as defined in Section 2.2-4301 of the Virginia Public Procurement Act. All shipping costs shall be included in the cost of equipment and no additional shipping charges shall be incurred at the time of invoicing.

Section 16

(NEW) PURCHASE REPORT

The Contractor shall furnish the Division of Purchases and Supply reports of the total dollar volume of purchases by ordering Agency and the total number of each contract item ordered under this contract with dollar amounts on a quarterly basis, i.e., 1st quarter = July, August & September - submit report by October 30th; 2nd quarter = October, November & December - submit report by January 30th.

Section 17

MINIMUM ORDERS

There will be no minimum order requirements under this contract.

Section 18

PRICE CHANGES PART 1

Price adjustments may be permitted only for changes in the Contractor's cost of materials not to exceed the increase in the following index/indices: Producer's price index will be used as a guide in determining adjustments. No price increases will be authorized for 365 calendar days after the effective date of the contract. Price escalation may be permitted only at the end of this period and each 365 days thereafter and only where verified to the satisfaction of the purchasing office. However, "across the board" price decreases are subject to implementation at any time and shall be immediately conveyed to the Commonwealth.

Section 19

PRICE CHANGES PART 2

The Contractor shall document the amount and proposed effective date of any general change in the price of materials. Documentation shall be supplied with the Contractor's request for increase which will: (1) verify that the requested price increase is general in scope and not applicable just to the Commonwealth of Virginia; and (2) verify the amount or percentage of increase which is being passed on to the Contractor by the Contractor's suppliers. The purchasing office will notify the using agencies and Contractor in writing of the effective date of any increase which it approves. However, the Contractor shall fill all purchase orders received prior to the effective date of the price adjustment at the old contract prices. The Contractor is further advised that decreases which affect the cost of materials are required to be communicated immediately to the purchasing office.

Section 20

CANCELLATION OF CONTRACT

The purchasing agency reserves the right to cancel and terminate any resulting contract, in part or in whole, without penalty, upon 60 days written notice to the Contractor. In the event the initial contract period is for more than 12 months, the resulting contract may be terminated by either party, without penalty, after the initial 12 months of the contract period upon 60 days written notice to the other party. Any contract cancellation notice shall not relieve the Contractor of the obligation to deliver and/or perform on all outstanding orders issued prior to the effective date of cancellation.

Section 21

QUANTITIES

Any quantities (if any) set forth in this solicitation are estimates only, and the Contractor shall supply at bid prices actual quantities as ordered, regardless of whether such total quantities are more or less than those shown.

Section 22

AUDIT

The contractor shall retain all books, records, and other documents relative to this contract for five (5) years after final payment, or until audited by the Commonwealth of Virginia, whichever is sooner. The agency, its authorized agents, and/or state auditors shall have full access to and the right to examine any of said materials during said period.

Section 23

AVAILABILITY OF FUNDS

It is understood and agreed between the parties herein that the agency shall be bound hereunder only to the extent of the funds available or which may hereafter become available for the purpose of this agreement.

Section 24

RETURN POLICY

Exchange for credit may be accomplished by ordering agencies consistent with the contractor's published return goods policy. A copy of bidder's published return goods policy should accompany the bid. Failure to submit the policy may be cause for rejection of the bid.

Section 25

TRAINING AND INSTALLATION

The awarded Contractor(s) shall provide on-site In-service training to the personnel of the ordering Agency to ensure proper use of equipment. Additional training shall be made available at the request of the ordering agency, led by a sales representative and/or one instructional video/DVD in English, provided at no additional cost to the Commonwealth. Training shall be held at the ordering Agency facility. Price of equipment shall include installation and assembly of patient lift and transfer systems.

Section 26

WARRANTY PART 1

All materials and equipment shall be fully guaranteed against defects in material and workmanship for a period of 365 days following date of delivery. Should any defect be noted by the owner, the Purchasing Office will notify the Contractor of such defect or nonconformance. Notification will state either (1) that the Contractor shall replace or correct, or (2) the owner does not require replacement or correction, but an equitable adjustment to the contract price will be negotiated.

Section 27

WARRANTY PART 2

If the Contractor is required to correct or replace, it shall be at no cost to the Commonwealth and shall be subject to all provisions of this clause to the same extent as materials initially delivered. If the Contractor fails or refuses to replace or correct the deficiency, the office issuing the purchase order may have the materials corrected or replaced with similar items and charge the Contractor the costs occasioned thereby or obtain an equitable adjustment in the contract price.

Section GEN

GENERAL TERMS AND CONDITIONS

VENDORS MANUAL: This solicitation is subject to the provisions of the Commonwealth of Virginia Vendors Manual and any changes or revisions thereto, which are hereby incorporated into this contract in their entirety. The procedure for filing contractual claims is in section 7.19 of the Vendors Manual. A copy of the manual is normally available for review at the purchasing office and is accessible on the Internet at www.dgs.state.va.us/dps under "Manuals."

APP. LAWS AND COURTS

APPLICABLE LAWS AND COURTS: This solicitation and any resulting contract shall be governed in all respects by the laws of the Commonwealth of Virginia and any litigation with respect thereto shall be brought in the courts of the Commonwealth. The agency and the contractor are encouraged to resolve any issues in controversy arising from the award of the contract or any contractual dispute using Alternative Dispute Resolution (ADR) procedures (Code of Virginia, § 2.2-4366). ADR procedures are described in Chapter 9 of the Vendors Manual. The contractor shall comply with all applicable federal, state and local laws, rules and regulations.

ANTI-DISCRIMINATION (1 of 2)

ANTI-DISCRIMINATION (part 1 of 2): By submitting their (bids/proposals), (bidders/offerors) certify to the Commonwealth that they will conform to the provisions of the Federal Civil Rights Act of 1964, as amended, as well as the Virginia Fair Employment Contracting Act of 1975, as amended, where applicable, the Virginians With Disabilities Act, the Americans With Disabilities Act and § 2.2-4311 of the Virginia Public Procurement Act (VPPA). If the award is made to a faith-based organization, the organization shall not discriminate against any recipient of goods, services, or disbursements made pursuant to the contract on the basis of the recipient's religion, religious belief, refusal to participate in a religious practice, or on the basis of race, age, color, gender or national origin and shall be subject to the same rules as other organizations that contract with public bodies to account for the use of the funds provided; however, if the faith-based organization segregates public funds into separate accounts, only the accounts and programs funded with public funds shall be subject to audit by the public body. (Code of Virginia, § 2.2-4343.1E). (continued on part 2)

ANTI-DISCRIMINATION (2 of 2)

ANTI-DISCRIMINATION (part 2 of 2): In every contract over \$10,000 the provisions in 1. and 2. below apply: 1.) During the performance of this contract, the contractor agrees as follows: (a.) The contractor will not discriminate against any employee or applicant for employment because of race, religion, color, sex, national origin, age, disability, or any other basis prohibited by state law relating to discrimination in employment, except where there is a bona fide occupational qualification reasonably necessary to the normal operation of the contractor. The contractor agrees to post in conspicuous places, available to employees and applicants for employment, notices setting forth the provisions of this nondiscrimination clause. (b.) The contractor, in all solicitations or advertisements for employees placed by or on behalf of the contractor, will state that such contractor is an equal opportunity employer. (c.) Notices, advertisements and solicitations placed in accordance with federal law, rule or regulation shall be deemed sufficient for the purpose of meeting these requirements. 2.) The contractor will include the provisions of 1. above in every subcontract or purchase order over \$10,000, so that the provisions will be binding upon each subcontractor or vendor.

ETHICS IN PUBLIC CONTRACTING

ETHICS IN PUBLIC CONTRACTING: By submitting their (bids/proposals), (bidders/offerors) certify that their (bids/proposals) are made without collusion or fraud and that they have not offered or received any kickbacks or inducements from any other (bidder/offeror), supplier, manufacturer or subcontractor in connection with their (bid/proposal), and that they have not conferred on any public employee having official responsibility for this procurement transaction any payment, loan, subscription, advance, deposit of money, services or anything of more than nominal value, present or promised, unless consideration of substantially equal or greater value was exchanged.

IMMIGRATION REFORM

IMMIGRATION REFORM AND CONTROL ACT OF 1986: By submitting their (bids/proposals), (bidders/offerors) certify that they do not and will not during the performance of this contract employ illegal alien workers or otherwise violate the provisions of the federal Immigration Reform and Control Act of 1986.

DEBARMENT STATUS

DEBARMENT STATUS: By submitting their (bids/proposals), (bidders/offerors) certify that they are not currently debarred by the Commonwealth of Virginia from submitting bids or proposals on contracts for the type of goods and/or services covered by this solicitation, nor are they an agent of any person or entity that is currently so debarred.

ANTITRUST

ANTITRUST: By entering into a contract, the contractor conveys, sells, assigns, and transfers to the Commonwealth of Virginia all rights, title and interest in and to all causes of action it may now have or hereafter acquire under the antitrust laws of the United States and the Commonwealth of Virginia, relating to the particular goods or services purchased or acquired by the Commonwealth of Virginia under said contract.

MANDATORY USE OF STATE FORM

MANDATORY USE OF STATE FORM AND TERMS AND CONDITIONS FOR IFB's: Failure to submit a bid on the official state form provided for that purpose shall be a cause for rejection of the bid. Modification of or additions to any portion of the Invitation for Bids may be cause for rejection of the bid; however, the Commonwealth reserves the right to decide, on a case by case basis, in its sole discretion, whether to reject such a bid as nonresponsive. As a precondition to its acceptance, the Commonwealth may, in its sole discretion, request that the bidder withdraw or modify nonresponsive portions of a bid which do not affect quality, quantity, price, or delivery. No modification of or addition to the provisions of the contract shall be effective unless reduced to writing and signed by the parties.

CLARIFICATION OF TERMS

CLARIFICATION OF TERMS: If any prospective (bidder/offeror) has questions about the specifications or other solicitation documents, the prospective (bidder/offeror) should contact the buyer whose name appears on the face of the solicitation no later than five working days before the due date. Any revisions to the solicitation will be made only by addendum issued by the buyer.

PAYMENT (1 of 3)

PAYMENT (part 1 of 3): To Prime Contractor: a.) Invoices for items ordered, delivered and accepted shall be submitted by the contractor directly to the payment address shown on the purchase order/contract. All invoices shall show the state contract number and/or purchase order number; social security number (for individual contractors) or the federal employer identification number (for proprietorships, partnerships, and corporations). b.) Any payment terms requiring payment in less than 30 days will be regarded as requiring payment 30 days after invoice or delivery, whichever occurs last. This shall not affect offers of discounts for payment in less than 30 days, however. c.) All goods or services provided under this contract or purchase order, that are to be paid for with public funds, shall be billed by the contractor at the contract price, regardless of which public agency is being billed. d.) The following shall be deemed to be the date of payment: the date of postmark in all cases where payment is made by mail, or the date of offset when offset proceedings have been instituted as authorized under the Virginia Debt Collection Act. e.) Unreasonable Charges. Under certain emergency procurements and for most time and material purchases, final job costs cannot be accurately determined at the time orders are placed.(Continued on part 2)

PAYMENT (2 of 3)

PAYMENT (part 2 of 3): In such cases, contractors should be put on notice that final payment in full is contingent on a determination of reasonableness with respect to all invoiced charges. Charges

which appear to be unreasonable will be researched and challenged, and that portion of the invoice held in abeyance until a settlement can be reached. Upon determining that invoiced charges are not reasonable, the Commonwealth shall promptly notify the contractor, in writing, as to those charges which it considers unreasonable and the basis for the determination. A contractor may not institute legal action unless a settlement cannot be reached within thirty (30) days of notification. The provisions of this section do not relieve an agency of its prompt payment obligations with respect to those charges which are not in dispute (Code of Virginia, § 2.2-4363). 2. To Subcontractors: a.) A contractor awarded a contract under this solicitation is hereby obligated: (1) To pay the subcontractor(s) within seven (7) days of the contractor's receipt of payment from the Commonwealth for the proportionate share of the payment received for work performed by the subcontractor(s) under the contract; or (2) To notify the agency and the subcontractor(s), in writing, of the contractor's intention to withhold payment and the reason. (continued on part 3)

PAYMENT (3 of 3)

PAYMENT (part 3 of 3): b.) The contractor is obligated to pay the subcontractor(s) interest at the rate of one percent per month (unless otherwise provided under the terms of the contract) on all amounts owed by the contractor that remain unpaid seven (7) days following receipt of payment from the Commonwealth, except for amounts withheld as stated in (2) above. The date of mailing of any payment by U. S. Mail is deemed to be payment to the addressee. These provisions apply to each sub-tier contractor performing under the primary contract. A contractor's obligation to pay an interest charge to a subcontractor may not be construed to be an obligation of the Commonwealth. 3.) Each prime contractor who wins an award in which provision of a SWAM procurement plan is a condition to the award, shall deliver to the contracting agency or institution, on or before request for final payment, evidence and certification of compliance (subject only to insubstantial shortfalls and to shortfalls arising from subcontractor default) with the SWAM procurement plan. Final payment under the contract in question may be withheld until such certification is delivered and, if necessary, confirmed by the agency or institution, or other appropriate penalties may be assessed in lieu of withholding such payment..

PRECEDENCE OF TERMS

PRECEDENCE OF TERMS: The following General Terms and Conditions VENDORS MANUAL, APPLICABLE LAWS AND COURTS, ANTI-DISCRIMINATION, ETHICS IN PUBLIC CONTRACTING, IMMIGRATION REFORM AND CONTROL ACT OF 1986, DEBARMENT STATUS, ANTTITRUST, MANDATORY USE OF STATE FORM AND TERMS AND CONDITIONS, CLARIFICATION OF TERMS, PAYMENT shall apply in all instances. In the event there is a conflict between any of the other General Terms and Conditions and any Special Terms and Conditions in this solicitation, the Special Terms and Conditions shall apply.

QUALIFICATIONS

QUALIFICATIONS OF (BIDDERS/OFFERORS): The Commonwealth may make such reasonable investigations as deemed proper and necessary to determine the ability of the (bidder/offeror) to perform the services/furnish the goods and the (bidder/offeror) shall furnish to the Commonwealth all such information and data for this purpose as may be requested. The Commonwealth reserves the right to inspect (bidder's/offeror's) physical facilities prior to award to satisfy questions regarding the (bidder's/offeror's) capabilities. The Commonwealth further reserves the right to reject any (bid/proposal) if the evidence submitted by, or investigations of, such (bidder/offeror) fails to satisfy the Commonwealth that such (bidder/offeror) is properly qualified to carry out the obligations of the contract and to provide the services and/or furnish the goods contemplated therein.

TESTING AND INSPECTION

TESTING AND INSPECTION: The Commonwealth reserves the right to conduct any test/inspection it may deem advisable to assure goods and services conform to the specifications.

ASSIGNMENT OF CONTRACT

ASSIGNMENT OF CONTRACT: A contract shall not be assignable by the contractor in whole or in part without the written consent of the Commonwealth.

CHANGES TO CONTRACT (1 of 2)

CHANGES TO THE CONTRACT (part 1 of 2): Changes can be made to the contract in any of the following ways: (1.) The parties may agree in writing to modify the scope of the contract. An increase or decrease in the price of the contract resulting from such modification shall be agreed to by the parties as a part of their written agreement to modify the scope of the contract. (2.) The Purchasing Agency may order changes within the general scope of the contract at any time by written notice to the contractor. Changes within the scope of the contract include, but are not limited to, things such as services to be performed, the method of packing or shipment, and the place of delivery or installation. The contractor shall comply with the notice upon receipt. The contractor shall be compensated for any additional costs incurred as the result of such order and shall give the Purchasing Agency a credit for any savings. Said compensation shall be determined by one of the following methods: (2a.) By mutual agreement between the parties in writing; or (2b.) By agreeing upon a unit price or using a unit price set forth in the contract, if the work to be done can be expressed in units, and the contractor accounts for the number of units of work performed, subject to the Purchasing Agency's right to audit the contractor's records and/or to determine the correct number of units independently; or (continued on part 2)

CHANGES TO CONTRACT (2 of 2)

CHANGES TO THE CONTRACT (part 2 of 2): (2c.) By ordering the contractor to proceed with the work and keep a record of all costs incurred and savings realized. A markup for overhead and profit may be allowed if provided by the contract. The same markup shall be used for determining a decrease in price as the result of savings realized. The contractor shall present the Purchasing Agency with all vouchers and records of expenses incurred and savings realized. The Purchasing Agency shall have the right to audit the records of the contractor as it deems necessary to determine costs or savings. Any claim for an adjustment in price under this provision must be asserted by written notice to the Purchasing Agency within thirty (30) days from the date of receipt of the written order from the Purchasing Agency. If the parties fail to agree on an amount of adjustment, the question of an increase or decrease in the contract price or time for performance shall be resolved in accordance with the procedures for resolving disputes provided by the Disputes Clause of this contract or, if there is none, in accordance with the disputes provisions of the Commonwealth of Virginia Vendors Manual. Neither the existence of a claim nor a dispute resolution process, litigation or any other provision of this contract shall excuse the contractor from promptly complying with the changes ordered by the Purchasing Agency or with the performance of the contract generally.

DEFAULT

DEFAULT: In case of failure to deliver goods or services in accordance with the contract terms and conditions, the Commonwealth, after due oral or written notice, may procure them from other sources and hold the contractor responsible for any resulting additional purchase and administrative costs. This remedy shall be in addition to any other remedies which the Commonwealth may have.

TAXES

TAXES: Sales to the Commonwealth of Virginia are normally exempt from State sales tax. State sales and use tax certificates of exemption, Form ST-12, will be issued upon request. Deliveries against this contract shall usually be free of Federal excise and transportation taxes. The Commonwealth's excise tax exemption registration number is 54-73-0076K.

USE OF BRAND NAMES

USE OF BRAND NAMES: Unless otherwise provided in this solicitation, the name of a certain brand, make or manufacturer does not restrict (bidders/offerors) to the specific brand, make or manufacturer named, but conveys the general style, type, character, and quality of the article desired. Any article which the public body, in its sole discretion, determines to be the equal of that specified, considering quality, workmanship, economy of operation, and suitability for the purpose intended,

shall be accepted. The (bidder/offeror) is responsible to clearly and specifically identify the product being offered and to provide sufficient descriptive literature, catalog cuts and technical detail to enable the Commonwealth to determine if the product offered meets the requirements of the solicitation. This is required even if offering the exact brand, make or manufacturer specified. Normally in competitive sealed bidding only the information furnished with the bid will be considered in the evaluation. Failure to furnish adequate data for evaluation purposes may result in declaring a bid nonresponsive. Unless the (bidder/offeror) clearly indicates in its (bid/proposal) that the product offered is an equal product, such (bid/proposal) will be considered to offer the brand name product referenced in the solicitation.

TRANSPORTATION AND PACKAGING

TRANSPORTATION AND PACKAGING: By submitting their (bids/proposals), all (bidders/offerors) certify and warrant that the price offered for FOB destination includes only the actual freight rate costs at the lowest and best rate and is based upon the actual weight of the goods to be shipped. Except as otherwise specified herein, standard commercial packaging, packing and shipping containers shall be used. All shipping containers shall be legibly marked or labeled on the outside with purchase order number, commodity description, and quantity.

INSURANCE (1 of 3)

INSURANCE (part 1 of 3): By signing and submitting a bid or proposal under this solicitation, the bidder or offeror certifies that if awarded the contract, it will have the following insurance coverage at the time the contract is awarded. For construction contracts, if any subcontractors are involved, the subcontractor will have workers' compensation insurance in accordance with §§ 2.2-4332 and 65.2-800 et seq. of the Code of Virginia. The bidder or offeror further certifies that the contractor and any subcontractors will maintain this insurance coverage during the entire term of the contract and that all insurance coverage will be provided by insurance companies authorized to sell insurance in Virginia by the Virginia State Corporation Commission. (continued in part 2)

INSURANCE (2 of 3)

INSURANCE (part 2 of 3) MINIMUM INSURANCE COVERAGES AND LIMITS REQUIRED FOR MOST CONTRACTS: 1) Workers' Compensation - Statutory requirements and benefits. Coverage is compulsory for employers of three or more employees, to include the employer. Contractors who fail to notify the Commonwealth of increases in the number of employees that change their workers' compensation requirements under the Code of Virginia during the course of the contract shall be in noncompliance with the contract. 2) Employer's Liability - \$100,000. 3) Commercial General Liability - \$1,000,000 per occurrence. Commercial General Liability is to include bodily injury and property damage, personal injury and advertising injury, products and completed operations coverage. The Commonwealth of Virginia must be named as an additional insured and so endorsed on the policy 4) Automobile Liability - \$1,000,000 per occurrence. (Only used if motor vehicle is to be used in the contract.). (continued in part 3)

INSURANCE (3 of 3)

INSURANCE (part 3 of 3): NOTE: In addition, various Professional Liability/Errors and Omissions coverage are required when soliciting those services as follows: Profession/Service /Limits, Accounting /\$1,000,000 per occurrence, \$3,000,000 aggregate Architecture/\$2,000,000 per occurrence, \$6,000,000 aggregate, Asbestos Design, Inspection or Abatement Contractors/ \$1,000,000 per occurrence, \$3,000,000 aggregate, Health Care Practitioner (to include Dentists, Licensed Dental, Hygienists, Optometrists, Registered or Licensed, Practical Nurses, Pharmacists, Physicians, Podiatrists, Chiropractors, Physical Therapists, Physical Therapist Assistants, Clinical Psychologists, Clinical Social Workers, Professional Counselors, Hospitals, or Health Maintenance Organizations.) \$1,750,000 per occurrence, \$3,000,000 aggregate, (Limits increase each July 1 through fiscal year 2008, as follows: July 1, 2005 - \$1,800,000, July 1, 2006 - \$1,850,000, July 1, 2007 - \$1,925,000, July 1, 2008 - \$2,000,000. This complies with §8.01-581.15 of the Code of Virginia. Insurance/Risk Management /\$1,000,000 per occurrence, \$3,000,000 aggregate,

Landscape/Architecture/\$1,000,000 per occurrence, \$1,000,000 aggregate, Legal/\$1,000,000 per occurrence, \$5,000,000 aggregate. Professional Engineer/\$2,000,000 per occurrence, \$6,000,000 aggregate, Surveying/\$1,000,000 per occurrence, \$1,000,000 aggregate

ANNOUNCEMENT OF AWARD

ANNOUNCEMENT OF AWARD: Upon the award or the announcement of the decision to award a contract over \$50,000, as a result of this solicitation, the purchasing agency will publicly post such notice on the DGS/DPS eVA website (www.eva.state.va.us) for a minimum of 10 days.

DRUG-FREE WORKPLACE

DRUG-FREE WORKPLACE: During the performance of this contract, the contractor agrees to (i) provide a drug-free workplace for the contractor's employees; (ii) post in conspicuous places, available to employees and applicants for employment, a statement notifying employees that the unlawful manufacture, sale, distribution, dispensation, possession, or use of a controlled substance or marijuana is prohibited in the contractor's workplace and specifying the actions that will be taken against employees for violations of such prohibition; (iii) state in all solicitations or advertisements for employees placed by or on behalf of the contractor that the contractor maintains a drug-free workplace; and (iv) include the provisions of the foregoing clauses in every subcontract or purchase order of over \$10,000, so that the provisions will be binding upon each subcontractor or vendor. For the purposes of this section, "drug-free workplace" means a site for the performance of work done in connection with a specific contract awarded to a contractor, the employees of whom are prohibited from engaging in the unlawful manufacture, sale, distribution, dispensation, possession or use of any controlled substance or marijuana during the performance of the contract.

NONDISCRIMINATION

NONDISCRIMINATION OF CONTRACTORS: A bidder, offeror, or contractor shall not be discriminated against in the solicitation or award of this contract because of race, religion, color, sex, national origin, age, disability, faith-based organizational status, any other basis prohibited by state law relating to discrimination in employment or because the bidder or offeror employs ex-offenders unless the state agency, department or institution has made a written determination that employing ex-offenders on the specific contract is not in its best interest. If the award of this contract is made to a faith-based organization and an individual, who applies for or receives goods, services, or disbursements provided pursuant to this contract objects to the religious character of the faith-based organization from which the individual receives or would receive the goods, services, or disbursements, the public body shall offer the individual, within a reasonable period of time after the date of his objection, access to equivalent goods, services, or disbursements from an alternative provider.

eVA REGISTRATION (1 of 2)

eVA BUSINESS-TO-GOVERNMENT VENDOR REGISTRATION: The eVA Internet electronic procurement solution, web site portal www.eVA.virginia.gov streamlines and automates government purchasing activities in the Commonwealth. The eVA portal is the gateway for vendors to conduct business with state agencies and public bodies. All vendors desiring to provide goods and/or services to the Commonwealth shall participate in the eVA Internet e-procurement solution either through the eVA Basic Vendor Registration Service or eVA Premium Vendor Registration Service. All bidders or offerors must register in eVA; failure to register will result in the bid/proposal being rejected.

Commodity Information

Please see the attached Pricing Schedule.

MasterCare
Patient Equipment, Inc.
Integrity Bath
Equipment Price List

WHEN ORDERING A SYSTEM W/Console USE PART NUMBERS 805030/40 & 805050

| <u>Part #</u> | <u>Model</u> | <u>Description</u> | <u>Qty</u> | <u>Price</u> |
|---------------|--------------|---|------------|--------------|
| 805010 | MB-80 (RH) | Integrity Tub Without Console (Reservoir) R.H. Door | (1) | \$9,134.88 |
| 805020 | MB-80 (LH) | Integrity Tub Without Console (Reservoir) L.H. Door | (1) | \$9,134.88 |
| 805030 | MB-80R (RH) | Integrity Tub Set Up For Console (Reservoir) R.H. Door | (1) | \$5,645.76 |
| 805040 | MB-80R (LH) | Integrity Tub Set Up For Console (Reservoir) L.H. Door | (1) | \$5,645.76 |
| 805050 | MB-R | Console (Reservoir) for Integrity Tub | (1) | \$6,468.48 |
| 805060 | MT-80 | Lower Carrier Frame Without Scale | (1) | \$1,220.16 |
| 805070 | MT-80 | Lower Carrier Frame With Scale | (1) | \$3,562.56 |
| 805080 | MT-80 | Upper Chair Fixed Back | (1) | \$1,152.00 |
| 805090 | MT-80 | Upper Chair Reclinable Back | (1) | \$1,758.72 |
| 802050 | MB-VB | Vacuum Breaker Kit--Integrity W/O Console | (1) | \$334.08 |
| | | **Special California Compliant Installation Cost Per Unit (Includes disconnecting existing tub- remove to a location on site for customer to dispose of. Uncrate and move MasterCare system into place. Connect water/drain/electrical. Secure system to the floor, perform all adjustments, test and make ready for use. (Includes disposal of all crating materials.) | (1) | \$1,000.00 |

- Memo:** All of the above bathing systems have as standard:
1. Temperature controlled mixing valve, fill and shower flow control valves installed on the tub deck or console depending on model selected
 2. Adjustable BathAire System with Multiple Jets
 3. Disinfecting System
 4. Temperature Monitoring System
 5. Shower Wand
 6. 2" Pop-up Drain

The Integrity Bath is designed with backflow prevention and comply with UL 1795 Standards. However, some local areas have additional codes or different interpretations of existing codes we cannot possibly be aware of. In such cases, the contracting customer/installer is responsible for providing whatever additional plumbing/electrical is required to meet local code.

Terms: 50% Down, Net 30, 1 1/2% Over (Terms Subject To Change Based on Credit Rating)
 FOB Destination Prices Valid Through July 31, 2008

MasterCare
Patient Equipment, Inc.
"A" Series Entrée Bath
Equipment Price List

All "A" Series Entrée's Require A Mixing Control Package That Must Be Ordered Separately

| <u>Part #</u> | <u>Model</u> | <u>Description</u> | <u>Qty</u> | <u>Price</u> |
|---------------|--------------|---|------------|--------------|
| 605100 | MB-59-A | 59 1/2" Entrée Bath System Set Up for Alcove Installation. | (1) | \$7,780.80 |
| 605110 | MB-68-A | 67 1/2" Entrée Bath System 3 Sided Access--Standard Installation. | (1) | \$7,887.36 |
| 605115 | MB-68-A (XL) | 75 1/2" Entrée Bath System--Extended Length 3 Sided Access--Standard Installation. | (1) | \$8,623.68 |
| 605095 | MB-Scale | Entrée Bath Scale (Not available with alcove models) | (1) | \$2,188.80 |
| 605125 | MB-VA | 30 GPM Mixing/Flow Control Valve | (1) | \$954.24 |
| 606040 | MB-DC | Dual Controls (BathAire & Door) | (1) | \$154.08 |
| 602050 | MB-VB | Vacuum Breaker Kit (Entrée "A" Models) | (1) | \$315.36 |
| | | **Special California Compliant Installation Cost Per Unit (Includes disconnecting existing tub- remove to a location on site for customer to dispose of. Uncrate and move MasterCare system into place. Connect water/drain/electrical. Secure system to the floor, perform all adjustments, test and make ready for use. (Includes disposal of all crating materials.) | (1) | \$1,000.00 |

Items Below this Line Are Special Order -- Requiring 6 - 8 Weeks Lead Time. (Check with factory for exact lead time)

| | | | | |
|--------|---------------|---|-----|------------|
| 605140 | MB-68-AH | 63 1/2" Entrée Bath System For Head End Corner Installation. | (1) | \$7,887.36 |
| 605141 | MB-68-AH (XL) | 69 1/2" Entrée Bath System --Extended Length For Head End Corner Installation. | (1) | \$8,623.68 |
| 605160 | MB-68-AF | 63 1/2" Entrée Bath System For Foot End Corner Installation. | (1) | \$7,887.36 |
| 605161 | MB-68-AF (XL) | 69 1/2" Entrée Bath System --Extended Length For Foot End Corner Installation. | (1) | \$8,623.68 |

Memo: All of the above bathing systems have as standard:

- | | |
|----------------------------------|--|
| 1. Power Door | 2. Adjustable BathAire System with Multiple Jets |
| 3. Temperature monitoring system | 4. Shower Wand |
| 5. 2" Pop-up Drain | |

The Entrée Bath is designed with backflow prevention and comply with UL 1795 Standards. However, some local areas have additional codes or different interpretations of existing codes that we cannot possibly be aware of. In such cases, the customer/installer is responsible for providing whatever additional plumbing/electrical is required to meet local codes.

Terms: 50% Down, Net 30, 1 1/2% Over (Terms Subject To Change Based on Credit Rating) PriceMBA 7/01/04
 FOB Destination Prices Valid Through July 31, 2008

MasterCare
Patient Equipment, Inc.
"AV" Series Entree Bath--With Built-In Plumbing Package
Equipment Price List

| <u>Part #</u> | <u>Model</u> | <u>Description</u> | <u>Qty</u> | <u>Price</u> |
|---|----------------|---|------------|--------------|
| 605010 | MB-59-AV | 59 1/2" Entrée Bath System Set Up for Alcove Installation. | (1) | \$9,302.40 |
| 605020 | MB-68-AV | 67 1/2" Entrée Bath System 3 Sided Access--Standard Installation. | (1) | \$9,408.00 |
| 605040 | MB-68-AV (XL) | 73 1/2" Entrée Bath System--Extended Length 3 Sided Access--Standard Installation. | (1) | \$10,144.32 |
| 605030 | MB-68-AVI | 69 1/2" Entrée Bath System Set Up for Island or Peninsula Installation. | (1) | \$10,281.60 |
| 605090 | MB-68-AVI (XL) | 75 1/2" Entrée Bath System--Extended Length Set Up for Island or Peninsula Installation. | (1) | \$11,123.52 |
| 606040 | MB-DC | Dual Controls (BathAire & Door) | (1) | \$154.08 |
| 605095 | MB-Scale | Entrée Bath Scale (Not available with alcove models) | (1) | \$2,188.80 |
| 602051 | MB-VB | Vacuum Breaker Kit (Entrée "AV" Models) | (1) | \$334.08 |
| | | **Special California Compliant Installation Cost Per Unit (Includes disconnecting existing tub- remove to a location on site for customer to dispose of. Uncrate and move MasterCare system into place. Connect water/drain/electrical. Secure system to the floor, perform all adjustments, test and make ready for use. (Includes disposal of all crating materials.) | (1) | \$1,000.00 |
| Items Below this Line Are Special Order -- Requiring 6 - 8 Weeks Lead Time. (Check with factory for exact lead time) | | | | |
| 605050 | MB-68-AVH | 63 1/2" Entrée Bath System For Head End Corner Installation. | (1) | \$9,408.00 |
| 605060 | MB-68-AVH (XL) | 69 1/2" Entrée Bath System --Extended Length For Head End Corner Installation. | (1) | \$10,144.32 |
| 605070 | MB-68-AVF | 63 1/2" Entrée Bath System For Foot End Corner Installation. | (1) | \$9,408.00 |
| 605080 | MB-68-AVF (XL) | 69 1/2" Entrée Bath System --Extended Length For Foot End Corner Installation. | (1) | \$10,144.32 |

Memo: All of the above bathing systems have as standard:
1. Fill and Shower Flow Control Valves Installed on the Tub Deck
2. Power Door
3. Adjustable BathAire System with Multiple Jets
4. Temperature Monitoring System
5. 2" Pop-up Drain
6. Shower Wand

The Entrée Bath is designed with backflow prevention and comply with UL 1795 Standards. However, some local areas have additional codes or different interpretations of existing codes that we cannot possibly be aware of. In such cases, the customer/installer is responsible for providing whatever additional plumbing/electrical is required to meet local codes.

Terms: 50% Down, Net 30, 1 1/2% Over (Terms Subject To Change Based on Credit Rating)
FOB Destination Prices Valid Through July 31, 2006 PriceMBAV 7/01/04

MasterCare
Patient Equipment, Inc.
Malibu Recumbent Bathing System
Equipment Price List

The Malibu Recumbent Bath Requires A Mixing Control Package That Must Be Ordered Separately

| <u>Part #</u> | <u>Model</u> | <u>Description</u> | <u>Qty</u> | <u>Price</u> |
|---------------|--------------|---|------------|--------------|
| 708010 | MB-70-FH | MasterCare Recumbent Bath Fixed Height | (1) | \$7,171.20 |
| 708030 | ML-70-A | MasterCare Stretcher Lift | (1) | \$5,184.00 |
| 708040 | ML-70-A | MasterCare Stretcher Lift With Scale | (1) | \$6,842.88 |
| 605125 | MB-VA | 30 GPM Mixing/Flow Control Valve Package | (1) | \$954.24 |
| | | Installation Cost Per Unit (Includes disconnecting existing tub-remove to a location on site for customer to dispose of. Uncrate and move MasterCare system into place. Connect water/drain/electrical. Secure system to the floor, perform all adjustments, test and make ready for use. (Includes disposal of all crating materials.) | (1) | \$1,000.00 |

- Memo:** All of the above bathing systems have as standard:
1. Adjustable BathAire System with Multiple Jets
 2. Temperature Monitoring System
 3. Shower Supply Elbow, Shower Wand, 8 Foot Hose & Holder
 4. Back Flow Prevention
 5. 2" Pop-up Drain

The Malibu Recumbent bath is designed to meet most plumbing codes. However, some local areas have additional codes or different interpretations of existing codes that we cannot possibly be aware of. In such cases, the customer/installer is responsible for providing whatever additional plumbing/electrical is required to meet local codes.

Terms: 50% Down, Net 30, 1 1/2% Over (Terms Subject To Change Based on Credit Rating)
 FOB Destination -- Prices Valid Through July 31, 2008

Note: For custom orders or modifications to the stretcher -- call for quote.

BARRIER FREE ACCESS



Ambulatory Walk-ins



Sliding Transfers




Interfaces with Most Modern lifts

ASK US ABOUT THE OTHER SYSTEMS IN OUR LINE



Front Entry: Integrity Bath
Patent No. 6,766,543 B1

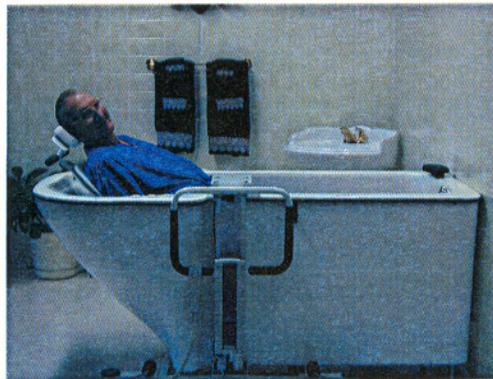

Malibu Recumbent Bath

MasterCare Patient Equipment, Inc.
2071 14th Avenue, PO Box 1435
Columbus, NE 68601-1435
Phone (800) 798-5867
Fax (402) 563-9102
E-mail: mastercarepeinc@frontiernet.net
Website: www.mastercarebath.net

MasterCare: Offering luxury, relaxation and comfort with safety, dignity and peace of mind through affordable bathing/showering solutions.


MasterCare

Patient Equipment, Inc.

ENTREE BATH



Superior Concepts in bathing to meet the needs of your residents and facility.

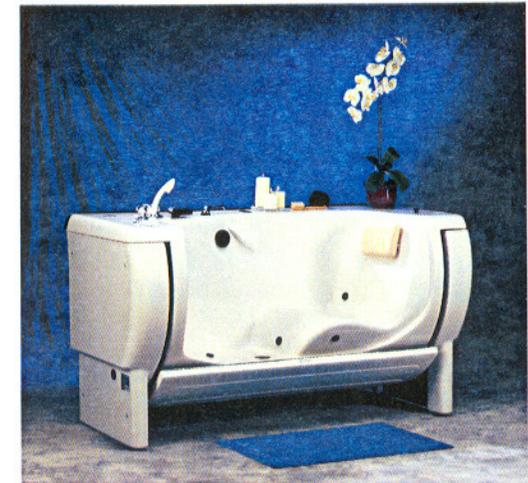


FEATURES OF THE **MasterCare**

ENTREE BATH

1. "Home-like" tub that creates a spa environment in your bathing area, making daily cleaning a safe and soothing experience.
2. "Barrier Free Access" side opening allows the wide, comfortable seat to extend over the floor surface. This cantilevered design provides easy access for ambulatory walk-ins, sliding transfers and interfaces with most modern lifts.
3. Easy "Push of a button" powered rotating door system that self-stores under the tub when open. There are NO obstructions to your transfer since the door extends the full length of the tub interior.
4. Simple push button controls allow your residents their independence or positioned for your caregiver's convenience.
5. Special safety controls prevent accidental opening of the tub when in use.
6. Fast fill temperature controlled water supply is achieved with an anti-scald thermoscopic mixing valve. Warm air keeps your resident comfortable while filling and draining.
7. XL version is a full six (6) inches longer in the interior of the tub, making it the longest side entry tub on the market.
8. Self-storing shower wand, variable speed BathAire^(SM) hydromassage and temperature monitoring system standard.
9. Easy to operate, clean and maintain.

USER FRIENDLY CONTROLS

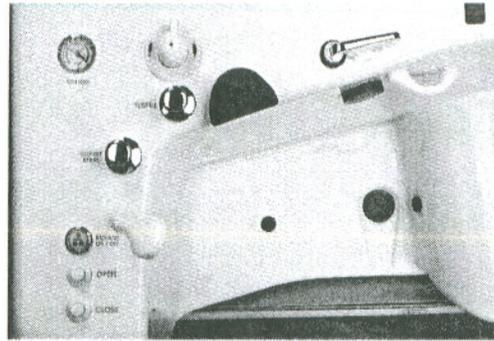


MasterCare Entree Bathing system is available in a variety of installation configurations to ensure the best possible working environment for your bathing area. **Room drawings can be prepared by request at no charge to ensure that the system will fit in your bathing area.**

Simple push-button door controls ensure proper seal each and every time.



**Call MasterCare @
800-798-5867 or visit us on the
web at: www.mastercarebath.net**


BATHAIRE^(SM)

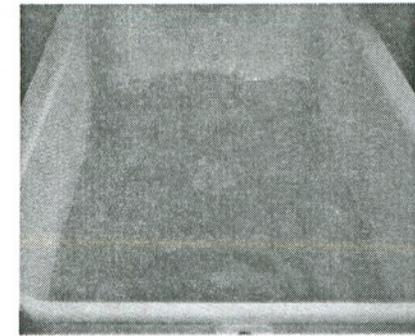

BathAire^(SM) patient cleaning system with self-sealing valves has the following advantages over conventional whirlpool bathing systems.

1. Self-sealing air valve outlets inhibits contaminated water from entering the internal air system significantly reducing the potential for cross-contamination.
2. BathAire^(SM) eliminates the extra time/labor, hot water and cleaner/disinfectant needed to sanitize and back flush a whirlpool's plumbing system.
3. The warm air flows evenly through 4 jets with 6 ports each totaling 24-air openings to create a gentle, soothing bathing experience. This feature can be activated by the push of a button ensuring that your resident is warm and comfortable while the tub is filling or draining.
4. Comfortable, soothing hydromassage is created from full bottom to top distribution of BathAire^(SM) cleaning action.

Transferring is as easy as 1-2-3

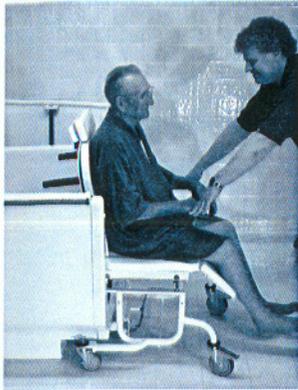


Step One:

Transfer system guides into place and attaches to the rail system easily and efficiently.



Step Two:

Chair glides on rail system to position resident for bathing.

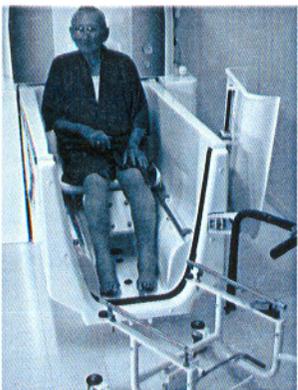


Step Three:

Transfer base is easily removed from system and out of caregiver's way using the armrest.

ASK US ABOUT THE OTHER SYSTEMS IN OUR LINE



Side Entry: Entrée Bath

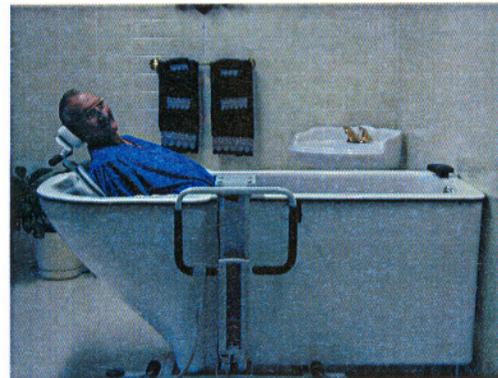

Malibu Recumbent Bath

MasterCare Patient Equipment, Inc.
2071 14th Avenue, PO Box 1435
Columbus, NE 68601-1435
Phone (800) 798-5867
Fax (402) 563-9102

E-mail: mastercarepeinc@frontiernet.net
Website: www.mastercarebath.net

MasterCare: Offering luxury, relaxation and comfort with safety, dignity and peace of mind through affordable bathing/showering solutions.

MasterCare

Patient Equipment, Inc.

INTEGRITY BATH



Superior concepts in bathing to meet the needs of your residents and facility.




Many options available to provide specialized care for multiple skill levels.

FEATURES OF THE MasterCare INTEGRITY BATH

1. Front entry system, with optional multi-position reclining chair. Ergonomic design of chair provides the deepest immersion for this type system on the market today.
2. Standard head rest aids your resident and bath aide in shampooing of hair, no related neck strain.
3. Chair locks to base for wheelchair like transport and no lift transfer for bathing. Your residents need only be transferred once.
4. Easy operational door locks in place for proper seal each and every time, reducing staff training.
5. Leg rest lifts your resident's legs for transport and reduces stress for the bath aide.
6. Reservoir can be pre-filled before your resident is brought to bathing area and during bathing for next bath, expediting the bathing process, saving time and money. Bath fill takes only 90 seconds.
7. Low profile side's aide caregiver in bathing procedures reducing fatigue and back strain.
8. Auto disinfecting, variable speed BathAire^(SM) hydromassage and temperature monitoring system standard.


USER FRIENDLY CONTROLS

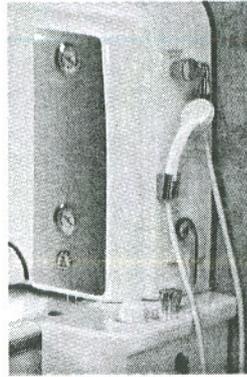

Separate, easy to use controls for bathing and disinfecting. Antiscald mixing valve, shower wand, tub fill and BathAire controls easily accessible to caregiver.


MasterCare Integrity Bathing system can be ordered with a right or left hinge door to ensure the best possible working environment for your bathing area. **Room drawings can be prepared by request at no charge to ensure that the system will fit in your allotted space.**

Simple door closure insures proper seal each and every time.

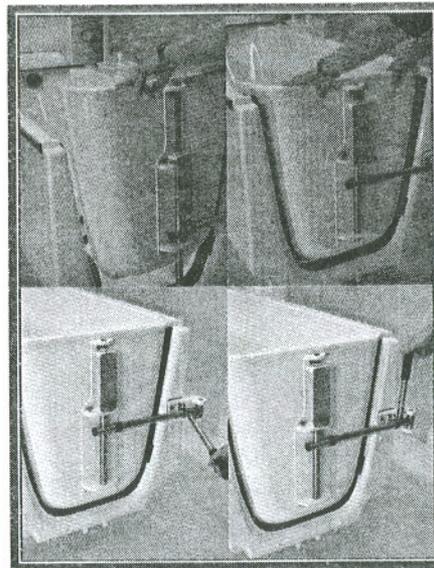

Patent No. 6,766,543 B1

BATHAIRE^(SM)

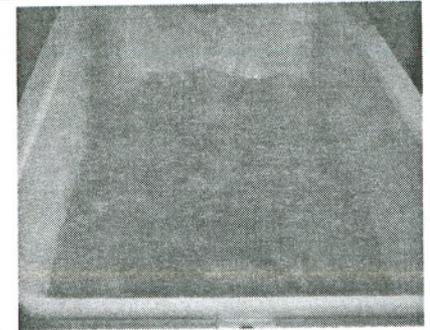


BathAire^(SM) patient cleaning system with self-sealing valves has the following advantages over conventional whirlpool bathing systems.

1. Self-sealing air valve outlets inhibits contaminated water from entering the internal air system significantly reducing the potential for cross-contamination.
2. BathAire^(SM) eliminates the extra time/labor, hot water and cleaner/disinfectant needed to sanitize and back flush a whirlpool's internal plumbing system.
3. The warm air flows evenly through 4 jets with 6 ports each totaling 24-air openings to create a gentle, soothing bathing experience. This feature can be activated by the push of a button, ensuring that your resident is warm and comfortable while the tub is filling or draining.
4. Comfortable, soothing hydromassage is created from full bottom to top distribution of BathAire^(SM) cleaning action.

MasterCare

STRETCHER LIFT FEATURES

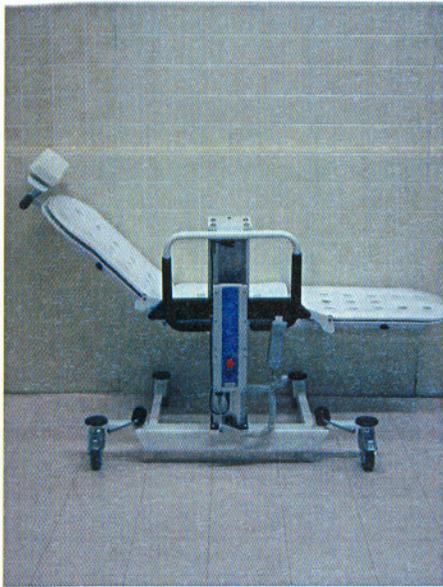

1. Unique low profile lift allows the attendant access to the resident from two sides.
2. Standard adjustable head rest aids your resident and bath aide in shampooing of hair, no related neck strain.
3. Hand held control easily operates the lift using one hand.
4. Optional scale available.
5. Four (4) inch rear swivel casters with brake, three (3) inch dual wheel swivel casters and caster guides at each end for straight steering down hallways.
6. Mattress pads standard, made of vinyl coated closed cell foam.
7. Rated to 350 lbs.

ASK US ABOUT THE OTHER
SYSTEMS IN OUR LINE



Side Entry: Entrée Bath



Front Entry: Integrity Bath
Patent No. 6,766,543 B1

MasterCare Patient Equipment, Inc.
2071 14th Avenue, PO Box 1435
Columbus, NE 68601-1435
Phone (800) 798-5867
Fax (402) 563-9102


E-mail: mastercarepeinc@frontiernet.net
Website: www.mastercarebath.net

**MasterCare: Offering luxury,
relaxation and comfort with
safety, dignity and peace of mind
through affordable
bathing/showering solutions.**

MasterCare

Patient Equipment, Inc.

MALIBU RECUMBENT BATH

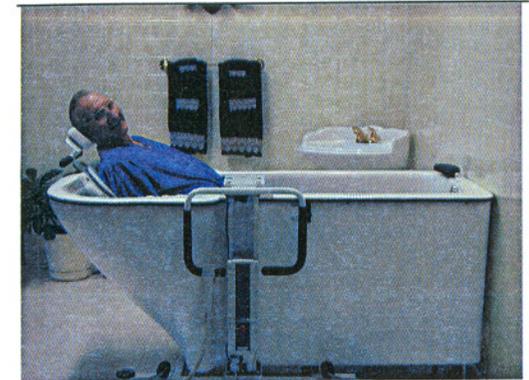

Superior concepts in bathing to
meet the needs of your residents
and facility.



Many options available to provide
specialized care for multiple skill
levels.

FEATURES OF THE **MasterCare** MALIBU RECUMBENT BATH


1. Recumbent system with inner tub shell design with the head end wider to improve ergonomic access to your resident.
2. Full range of height adjustments to facilitate low-level transfers.
3. Pre-fill before resident is brought to bathing area to expedite bathing process.
4. Full size bathing in a small area.
5. Adjusts to comfortable working height for caregiver to minimize back strain.
6. Non-institutional shape helps create normalized environment.
7. Variable speed BathAire^(SM) hydromassage and temperature monitoring system standard.




USER FRIENDLY CONTROLS



MasterCare Malibu Recumbent Bathing system can be ordered with fixed height or adjustable height to ensure the best possible working environment for your bathing area. **Room drawings can be prepared by request at no charge to ensure that the system will fit in your allotted space.**

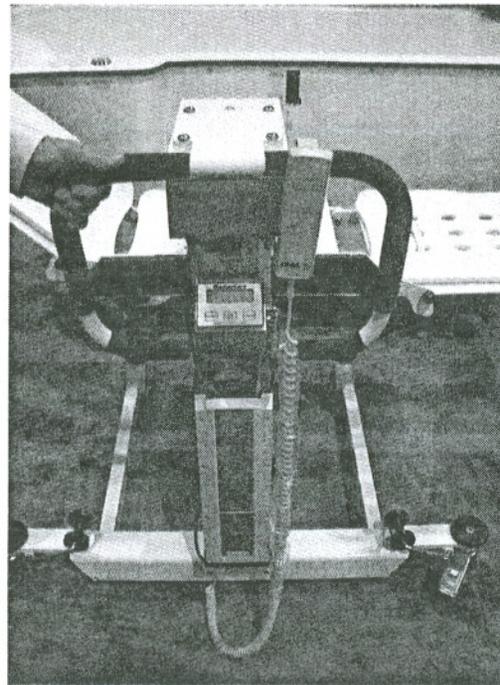

BATHAIRE^(SM)

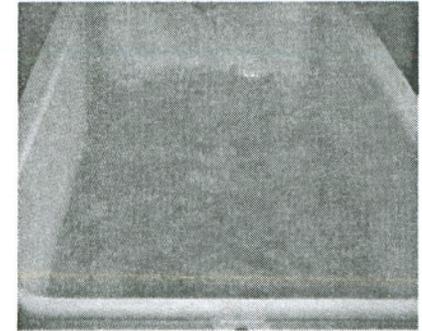

BathAire^(SM) patient cleaning system with self-sealing valves has the following advantages over conventional whirlpool bathing systems.

1. Self-sealing air valve outlets inhibits contaminated water from entering the internal air system significantly reducing the potential for cross-contamination.
2. BathAire^(SM) eliminates the extra time/labor, hot water and cleaner/disinfectant needed to sanitize and back flush a whirlpool's internal plumbing system.
3. The warm air flows evenly through 4 jets with 6 ports each totaling 24-air openings to create a gentle, soothing bathing experience. This feature can be activated by the push of a button, ensuring that your resident is warm and comfortable while the tub is filling or draining.
4. Comfortable, soothing hydromassage is created from full bottom to top distribution of BathAire^(SM) cleaning action.

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Entrée Bath

Architectural Specifications & Rough-In Information

Models: MB-59-A, MB-68-A, MB-68-AH & MB-68-AF, Including all XL Models

Dimensions:

| | | | | |
|-------|--------|--|-------|--------|
| Bath: | Width | [MB-59-A, MB-68-A, MB-68-AH, MB-68-AF (Including XL Models)] | 35" | Inches |
| | Length | [MB-59-A] | 59 ½" | Inches |
| | Length | [MB-68-A] | 67 ½" | Inches |
| | Length | [MB-68-AH, MB-68-AF] | 63 ½" | Inches |
| | Length | [MB-68-A(XL)] | 73 ½" | Inches |
| | Length | [MB-68-AH(XL), MB-68-AF(XL)] | 69 ½" | Inches |
| | Height | [MB-59-A, MB-68-A, MB-68-AH, MB-68-AF (Including XL Models)] | 40 ½" | Inches |

Specifications:

| | |
|-----------------------------------|--|
| Back Flow Prevention: | 1" Air gap for fill spout. Note: The factory provided Watts NLF-9 vacuum breaker for backflow prevention is the most widely accepted. Local codes may require changes, which is the responsibility of the local plumbing contractor. |
| BathAire ^(SM) Outlets: | 4 with 6 ports each for a total 24 warm air massage outlets. |
| Door Seal: | Tough, flexible vinyl cover and flange with closed cell foam core for long lasting durability. Highly resistant to oils, detergents and all water conditions. |
| Electrical: | Provide separate 120 V-AC, 60 HZ, 20 Amp. circuit and receptacle with in-line ground fault interrupter (not supplied) in accessible location. |
| Installation Time: | 1 hour |
| Motor Specs: | Door motor: 115 V., 4.2 Amps, 1/3 H.P. BathAire ^(SM) Motor: 120 V., 9.5 Amps. Variable speed with built-in 600 watt heating element for maximum comfort and control. |
| Room Size: | 5'11" wide x 9'7 ½" long minimum recommended for standard length; 6'5" wide x 10'1 ½" long minimum recommended for XL models. Can fit in smaller room; call MasterCare with dimensions. |
| Standards: | Tested and certified to Hydromassage Bathtubs, UL 1795, Third Edition. & Hydromassage Bathtub Appliances, CAN/CSA C22.2 No. 218.2-93. Compliant with chapters Comm 82-84, Wisconsin Administrative Code, and Chapters 145-160, Wisconsin Statutes. Comm 82.32 (4) (b) 2., Wis. Adm. Code based on the Wisconsin Statutes and the Wisconsin Administrative Code. Product File #20010143. FDA Establishment Registration No. 3003333691. |
| Switches: | Pneumatic and membrane. |
| Thermometer: | Analog temperature measurements. |
| Tub Entry: | Door full length of tub with tub seat extending over the floor surface. |
| Tub Fill/Shower: | Wall-mounted 30 GPM thermoscopic mixing valve with separate fill and shower flow control valves. |
| Tub Shell: | Sanitary gel-coated FRP (Fiberglass Reinforced Polymer). |
| Tub Water Use Gallonage: | 55 gallons under normal conditions. |
| Waste: | 2" PVC schedule 40 pipe. |
| Water Connection: | ½" & ¾" hose connections with shower & fill hoses supplied by manufacturer |
| Water Supply: | ¾" Copper hot and cold. Minimum of 45 PSI for hot and cold required. Maximum temperature of hot water supply 115° F or code, whichever is less. |
| Weight: | MB-59-A: Approx. 370 lbs, MB-68-A: Approx. 420 lbs, MB-68-A, MB-68-AF: Approx. 405 lbs, MB-68-A(XL): Approx. 460 lbs., MB-68-AH(XL) & MB-68-AF(XL): Approx. 445 lbs. |

Warning: 1) Risk of electrical shock; Disconnect electric power source before installation and subsequent servicing. 2) An equipment grounding terminal is provided in the field wiring compartment. To reduce the risk of electrical shock, this terminal must be connected to the grounding means provided in the electric supply panel with a conductor equivalent in size to the circuit conductors supplying this equipment. 3) Install this unit in accordance with the U.S. National Electrical Code in the U.S.A and the Canadian Electrical Code, Part I in Canada.

Other Precautions: Install to permit access for servicing.

Entrée A Series Specs 4/26/06
Rev. #1

2071 14th Avenue · PO Box 1435 · Columbus, NE 68601

Phone: 800.798.5867 · Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Entrée Bath

Architectural Specifications & Rough-In Information

Models: MB-59-AV, MB-68-AV, MB-68-AVH, MB-68-AVF & MB-68-AVI, Including all XL Models

Dimensions:

| | | | | |
|--------|-----------------|--|---------|--------|
| Bath: | Width | [MB-59-AV, MB-68-AV, MB-68-AVH, MB-68-AVF (Including XL models)] | 35" | Inches |
| | Width | [MB-68-AVI(XL)] | 38 1/2" | Inches |
| | Length | [MB-59-AV] | 59 1/2" | Inches |
| | Length | [MB-68-AV] | 67 1/2" | Inches |
| | Length | [MB-68-AVH, MB-68-AVF] | 63 1/2" | Inches |
| | Length | [MB-68-AVI] | 69 1/2" | Inches |
| | Length | [MB-68-AV(XL)] | 73 1/2" | Inches |
| | Length | [MB-68-AVH(XL), AVF(XL)] | 69 1/2" | Inches |
| | Length | [MB-68-AVI(XL)] | 75 1/2" | Inches |
| | Height | [MB-68-AV(XL), AVH(XL), AVF(XL)] | 40 1/2" | Inches |
| Height | [MB-68-AVI(XL)] | 42 1/2" | Inches | |

Specifications:

| | |
|-----------------------------------|--|
| Back Flow Prevention: | Watts NLF-9 vacuum breaker for shower hose. Note: The factory provided backflow prevention is the most widely accepted. Local codes may require changes, which is the responsibility of the local plumbing contractor. |
| BathAire ^(SM) Outlets: | 4 with 6 ports each for a total 24 warm air massage outlets. |
| Door Seal: | Tough, flexible vinyl cover and flange with closed cell foam core for long lasting durability. Highly resistant to oils, detergents and all water conditions. |
| Electrical: | Provide separate 120 V-AC, 60 HZ, 20 Amp. circuit and receptacle with in-line ground fault interrupter (not supplied) in accessible location. |
| Installation Time: | 1 hour |
| Motor Specs: | Door motor: 115 V., 4.2 Amps, 1/3 H.P. BathAire ^(SM) Motor: 120 V., 9.5 Amps. Variable speed with built-in 600 watt heating element for maximum comfort and control. |
| Room Size: | 5' 11" wide x 9' 7 1/2" long minimum recommended for standard length; 6'5" wide x 10'1 1/2" long minimum recommended for XL models. Can fit in smaller room; call MasterCare with dimensions. |
| Standards: | Tested and certified to Hydromassage Bathtubs, UL 1795, Third Edition. & Hydromassage Bathtub Appliances, CAN/CSA C22.2 No. 218.2-93. Compliant with chapters Comm 82-84, Wisconsin Administrative Code, and Chapters 145-160, Wisconsin Statutes. Comm 82.32 (4) (b) 2., Wis. Adm. Code based on the Wisconsin Statutes and the Wisconsin Administrative Code. Product File #20010143. FDA Establishment Registration No. 3003333691. |
| Switches: | Pneumatic and membrane. |
| Thermometer: | Analog temperature measurements. |
| Tub Entry: | Door full length of tub with tub seat extending over the floor surface. |
| Tub Fill/Shower: | Deck-mounted 22 GPM thermoscopic mixing valve with separate fill and shower flow control valves. |
| Tub Shell: | Sanitary gel-coated FRP (Fiberglass Reinforced Polymer). |
| Tub Water Use Gallonage: | 55 gallons under normal conditions. |
| Waste: | 2" PVC schedule 40 pipe. |
| Water Connection: | 1/2" & 3/4" hose connections with shower & fill hoses supplied by manufacturer |
| Water Supply: | 3/4" Copper hot and cold. Minimum of 45 PSI for hot and cold required. Maximum temperature of hot water supply 115° F or code, whichever is less. |
| Weight: | MB-59-AV: Approx. 370 lbs., MB-68-AV: Approx. 420 lbs., MB-68-AVH & MB-68-AVF: Approx. 405 lbs., MB-68-AVI: Approx. 440 lbs., MB-68-AV(XL): Approx. 460 lbs., MB-68-AVH(XL) & MB-68-AVF(XL): Approx. 445 lbs., MB-68-AVI(XL): Approx. 480 lbs. |

Warning: 1) Risk of electrical shock; Disconnect electric power source before installation and subsequent servicing. 2) An equipment grounding terminal is provided in the field wiring compartment. To reduce the risk of electrical shock, this terminal must be connected to the grounding means provided in the electric supply panel with a conductor equivalent in size to the circuit conductors supplying this equipment. 3) Install this unit in accordance with the U.S. National Electrical Code in the U.S.A and the Canadian Electrical Code, Part I in Canada.

Other Precautions: Install to permit access for servicing.

Entrée AV Series Specs 4/26/06
Rev. #1

2071 14th Avenue · PO Box 1435 · Columbus, NE 68601

Phone: 800.798.5867 · Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Entrée Bath Scale

Specification Information

Model: MS-80

Specifications:

| | |
|-----------------------|---|
| Accuracy: | Within 0.1% of capacity. |
| Capacity: | The scale uses 2 - 200 kg., single point, aluminum loadcells with potted gages for moisture protection. The loadcells have matched output so that load cell exchange does not then necessitate calibration. |
| Display: | LCD with .60" high characters |
| Electronics: | Utilizes a microprocessor controlled digital electronics for reliable and trouble free operation. |
| Mechanical: | Electronics enclosure is stainless steel with plastic overlay. The loadcell supports are heavy gauge stainless steel. All fasteners are stainless steel. |
| Mode: | Pounds (lb.) and Kilograms (kg) |
| Power: | 4 AA alkaline batteries |
| Repeatability: | To within 1 displayed division. |
| Resolution: | The present resolution is .5 lb. If finer resolution is needed, it is factory programmable. |

Features:

- All functions are accessible to the user without opening the enclosure.
- Starting or zeroing the unit is done through a single touch pad located on the front of the enclosure.
- Mode change (lb. to kg. or kg. to lb.) requires the LB/KG pad to be held in for 3 seconds to prevent inadvertent mode changes.
- Stable readings are achieved through digital averaging. Hold is activated when weight fluctuations reach a predetermined range. The scale becomes active when that range is exceeded.
- Display turns off after two minutes of inactivity to conserve battery life. This is factory programmable if a different time is required.
- Battery exchange is easy with simple removal of the indicator cover.
- Calibration is digital and performed without having to physically access the electronics.

Entrée Scale Specs 9/27/04

2071 14th Avenue · PO Box 1435 · Columbus, NE 68601

Phone: 800.798.5867 · Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Integrity Bath

Architectural Specifications & Rough-In Information

Standard Tub Models MB-80, MB-80-C & MB-80-CR

Reservoir Tub Models MB-80-R, MB-80-RC & MB-80-RCR

Dimensions:

| | | | | |
|-------|-------------------|-----------|---------------------------------|---------|
| Bath: | Width: | Standard | (MB-80, MB-80-C & MB-80-CR) | 33 1/2" |
| | Width: | Reservoir | (MB-80-R, MB-80-RC & MB-80-RCR) | 52 1/2" |
| | Length: | Standard | (MB-80, MB-80-C & MB-80-CR) | 70 1/2" |
| | Length: | Reservoir | (MB-80-R, MB-80-RC & MB-80-RCR) | 80 1/2" |
| | Tub Rim Height: | | (All Models) | 35 3/4" |
| | Reservoir Height: | Reservoir | (MB-80-R, MB-80-RC & MB-80-RCR) | 67" |

Specifications:

| | | | |
|---|--|-----------------------------|----------|
| Back Flow Prevention: | 1" Air gap for tub fill, vacuum breaker for MB-80-R shower hoses. Watts N-9 double checks for MB-80 shower hoses. Note: The factory provided backflow prevention is the most widely accepted. Local codes may require changes, which is the responsibility of the local plumbing contractor. | | |
| BathAire ^(SM) Outlets: | 4 with 6 ports each for a total 24 warm air massage outlets. | | |
| Door Seal: | Closed cell black Neoprene sponge. Highly resistant to oils, detergents and all water conditions. | | |
| Electrical: | Provide separate 120 V-AC, 60 HZ, 15 Amp. circuit and receptacle with in-line ground fault interrupter (not supplied) in accessible location. | | |
| Installation Time: | 1 1/2 hours | Inspection and Adjustments: | 1/2 hour |
| Liquids Storage: | Located behind lockable service access doors. | | |
| Motor Specs: | BathAire ^(SM) Motor: 120 V., 9.5 Amps. Variable speed with built-in 600 watt heating element for maximum comfort and control. | | |
| Patent: | US 6,766,543 B1. | | |
| Room Size: | Standard Model (RH) 6' wide x 9'4" long; Reservoir model (RH) 6' wide x 10' long. Can fit in smaller room; call MasterCare with dimensions. | | |
| Service Access: | Controlled access through lockable service doors. | | |
| Standards: | Tested and certified to Hydromassage Bathtubs, UL 1795, Third Edition. & Hydromassage Bathtub Appliances, CAN/CSA C22.2 No. 218.2-93. Compliant with chapters Comm 82-84, Wisconsin Administrative Code, and Chapters 145-160, Wisconsin Statutes. Comm 82.32 (4) (b) 2., Wis. Adm. Code based on the Wisconsin Statutes and the Wisconsin Administrative Code. Product File #20010143. FDA Establishment Registration No. 3003333691. | | |
| Switches: | Pneumatic and membrane. | | |
| Thermometer: | Analog temperature measurements. | | |
| Tub Entry: | Door counter-balanced with simple guidance system for easy of operation. | | |
| Tub Fill/Shower: | On-board 30 GPM mixing valve on standard models, and 22 GPM mixing valve on reservoir models. | | |
| Tub Shell: | Sanitary gel-coated FRP (Fiberglass Reinforced Polymer). | | |
| Tub Water <small>Use Gallonage:</small> | 55 gallons under normal conditions. | | |
| Waste: | 2" PVC schedule 40 pipe. | | |
| Water Connection: | 3/4" & 3/4" hose swivel connections supplied by manufacturer | | |
| Water Supply: | 3/4" Copper hot and cold. Minimum of 45 PSI for hot and cold required. Maximum temperature of hot water supply 115° F or code, whichever is less. Shut off valves at unit supplied by local plumbing contractor. | | |
| Weight: | MB-80 (420 lbs), MB-80-C (480 lbs), MB-80-R (Tub 385 lbs, Reservoir 240 lbs), MB-80-RC (Tub 445 lbs, Reservoir 240 lbs), MT-80 Transfer system (120 lbs). | | |
| Warning: | 1) Risk of electrical shock; Disconnect electric power source before installation and subsequent servicing. 2) An equipment grounding terminal is provided in the field wiring compartment. To reduce the risk of electrical shock, this terminal must be connected to the grounding means provided in the electric supply panel with a conductor equivalent in size to the circuit conductors supplying this equipment. 3) Install this unit in accordance with the U.S. National Electrical Code in the U.S.A and the Canadian Electrical Code, Part I in Canada | | |

Integrity Specs
Rev 1
04/13/06

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Integrity Bath Transfer System & Scale

Specification Information

Models: MT-80, MS-80

Dimensions:

| | | | |
|-----------------|--|-------|--------|
| Transfer Chair: | Width | 26" | Inches |
| | Length | 36" | Inches |
| | Height (Top of Chair Back) | 42 ½" | Inches |
| | Height (Top of Seat) (Wheelchair Height) | 21" | Inches |

Transfer System Specifications:

| | |
|---------------------------|---|
| Adjustable Back: | Gas spring offers infinite adjustability. |
| Arm Rests: | Articulating arm rests. |
| Base Construction: | Powder coated aluminum, stainless steel and high impact polymers. |
| Capacity: | 500 lbs. |
| Casters: | Four (4) swivel casters, two (2) 5" with brakes and two (2) 4" without brakes. |
| Chair: | Powder coated aluminum, stainless steel and high impact polymers. |
| Comfort Pads: | Vinyl covered closed-cell foam. |
| Leg Rest: | Adjustable to four (4) positions with flow through holes for water circulation. |
| Weight: | 120 lbs. |

Scale Specifications:

| | |
|-----------------------|---|
| Accuracy: | Within 1% of capacity. |
| Capacity: | The scale uses 2 - 200 kg., single point, aluminum loadcells with potted gages for moisture protection. The loadcells have matched output so that load cell exchange does not then necessitate calibration. |
| Display: | LCD with .60" high characters |
| Electronics: | Utilizes a microprocessor controlled digital electronics for reliable and trouble free operation. |
| Mechanical: | Electronics enclosure is stainless steel with plastic overlay. The loadcell supports are heavy gauge stainless steel. All fasteners are stainless steel. |
| Mode: | Pounds (lb.) and Kilograms (kg) |
| Power: | 4 AA alkaline batteries |
| Repeatability: | To within 1 displayed division. |
| Resolution: | The present resolution is .5 lb. If finer resolution is needed, it is factory programmable. |

Transfer & Scale Specs
Rev 1
04/13/06

2071 14th Avenue • PO Box 1435 • Columbus, NE 68601

Phone: 800.798.5867 • Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Malibu Recumbent Bath

Architectural Specifications & Rough-In Information

Models: MB-70-FH & AH

Dimensions:

| | | | |
|--------------|--------------------------------|-------|--------|
| Bath: | Width | 36" | Inches |
| | Length | 71" | Inches |
| | Height (tub rim down position) | 33 ½" | Inches |
| | Height (tub rim up position) | 44" | Inches |

Specifications:

| | |
|---|--|
| Back Flow Prevention: | Air gap for fill spout. Note: The factory provided backflow prevention is the most widely accepted. Local codes may require changes, which is the responsibility of the local plumbing contractor. |
| BathAire^(SM) Outlets: | 4 with 6 ports each for a total 24 warm air massage outlets. |
| Battery: | 12 V, 12 Ah battery on an automatic charger system with 12 V output at .75 amps allows tub height to be adjusted during power supply interruptions. |
| Electrical: | Provide separate 115 V-AC, 60 HZ, 20 Amp. circuit and receptacle with in-line ground fault interrupter (not supplied) in accessible location. |
| Fixed Height: | Adjustment to floor option allows for lift base clearance of 5" or can be lowered all the way down to floor. |
| Height Adjustment: | Powered by four (4) oil hydraulic cylinders. |
| Hydraulics: | 12 VDC ignition protected bi-directional 3,000 PSI hydraulic pump. |
| Installation Time: | 1 hour |
| Motor Specs: | BathAire ^(SM) Motor: 115 V., 7.0 Amps, 1.3 H.P. Adjustable speed for maximum comfort and control. |
| Room Size: | 7' wide x 8' 10" long minimum recommended. Can fit in smaller room; call MasterCare with dimensions. |
| Switches: | Pneumatic and membrane. |
| Thermometer: | Analog temperature measurements. |
| Tub Fill/Shower: | Wall-mounted 30 GPM thermoscopic mixing valve with separate fill and shower flow control valves. |
| Tub Shell: | Sanitary gel-coated FRP (Fiberglass Reinforced Polymer). |
| Tub Water Use Gallonage: | 55 gallons |
| Waste: | 2" PVC schedule 40 pipe. |
| Water Connection: | ½" & ¾" hose connections with shower & fill hoses supplied by manufacturer. |
| Water Supply: | ¾" Copper hot and cold. Minimum of 30 PSI for hot and cold required. Maximum temperature of hot water supply 115° F or code, whichever is less. |
| Weight: | MB-70-FH & AH: 400 lbs. |

Malibu Specs 9/27/04

2071 14th Avenue · PO Box 1435 · Columbus, NE 68601

Phone: 800.798.5867 · Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net

MasterCare

Patient Equipment, Inc.

"ERGONOMIC AND ECONOMIC PATIENT CARE SOLUTIONS"

Malibu Recumbent Stretcher Lift and Scale

Specification Information

Models: ML-70-A, MS-80

Dimensions:

| | | |
|-------------|-----------------------------------|------------------------|
| ML-70 Lift: | Stretcher Platform with Head Rest | 69 ½" Long, 18 ¾" Wide |
| | Overall Width of Lift | 32" Inches |
| | Lift Base | 40" Long, 28 ½" Wide |
| | Travel (Stroke) Range | 19 ½" Up and Down |
| | Stretcher Platform | 36 ½" Up Position |
| | Bottom Height | 17 ½" Down Position |
| | Top of Column Height | 33 ½" Down Position |
| | | 53 ½" Up Position |

Stretcher Lift Specifications:

| | |
|----------------------|---|
| Battery: | 24 V output at 2.0 Ah, high capacity with over 60 cycles when fully charged. |
| Capacity: | 350 lbs. |
| Casters: | Four inch rear swivel casters with brake, three inch dual wheel swivel casters. |
| Comfort Pads: | Vinyl covered closed cell foam. |
| Construction: | 100% powder coated aluminum with stainless steel hardware. |
| Power: | 24 V DC actuator system for quiet, efficient operation. |
| Weight: | 175 lbs. Shipping |

Scale Specifications:

| | |
|-----------------------|---|
| Accuracy: | Within 0.1% of capacity. |
| Capacity: | The scale uses 2 - 200 kg., single point, aluminum loadcells with potted gages for moisture protection. The loadcells have matched output so that load cell exchange does not then necessitate calibration. |
| Display: | LCD with .60" high characters |
| Electronics: | Utilizes a microprocessor controlled digital electronics for reliable and trouble free operation. |
| Mechanical: | Electronics enclosure is stainless steel with plastic overlay. The loadcell supports are heavy gauge stainless steel. All fasteners are stainless steel. |
| Mode: | Pounds (lb.) and Kilograms (kg) |
| Power: | 4 AA alkaline batteries |
| Repeatability: | To within 1 displayed division. |
| Resolution: | The present resolution is .5 lb. If finer resolution is needed, it is factory programmable. |

Malibu Lift Specs 9/27/04

2071 14th Avenue · PO Box 1435 · Columbus, NE 68601

Phone: 800.798.5867 · Fax: 402.563.9102

E-mail: mastercarepeinc@frontiernet.net

Website: www.mastercarebath.net